

May 2020

PPE Catalog

JR

JR CAPITAL PARTNERS
— LLC —


Z&T Care Solutions

Products

- 3 Layer Disposable Mask
- KN95 Mask
- N95 Mask
- 3M 1860 Mask

Products

- Medical Gloves
- Covid 19 Rapid Test Kits
- Isolation Gowns
- Hand Sanitizer (6.7oz/14oz)
- Medical Face Shield

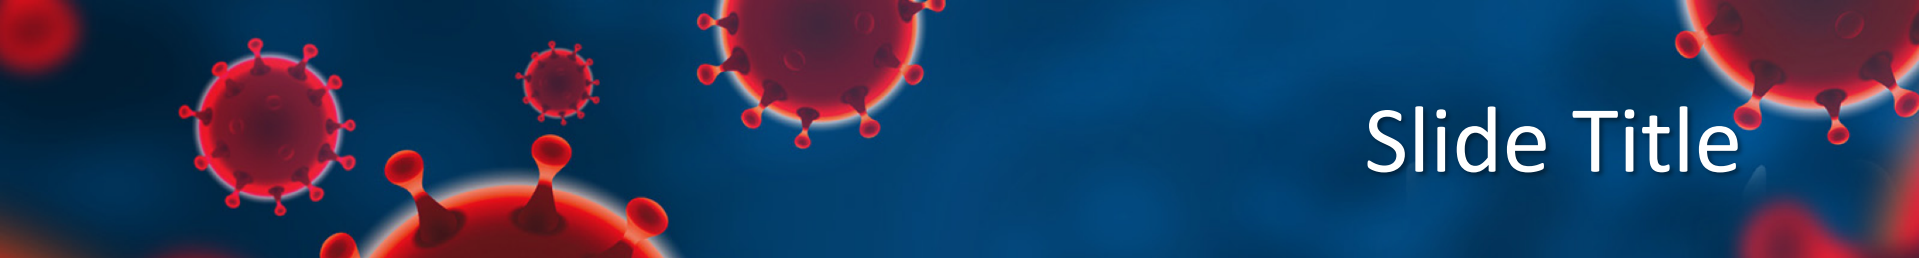

Slide Title





KN95 Surgical Particulate-filtering
Facial Protection Mask
FDA & CE Approved.
MOQ 100K
KN 95

Angaben Nr. PRD/7416249

DEKRA

Seite 6 von 6

Auftraggeber:
MA&L Engineering GmbH
Thomas Thring
Semenstr. 15b
40789 Monheim am Rhein
Germany

Anwesen:
DEKRA Testing and Certification GmbH
Hardenbergstr. 15
70565 Stuttgart
Deutschland

Auftrag zum Angebot Nr. PRD/7416249

Wir beauftragen gemäß dem vorliegenden Angebot unter Anerkennung der Allgemeinen Geschäftsbedingungen von DEKRA Testing and Certification GmbH die mit „X“ gekennzeichneten Positionen.

Folgende Positionen werden gemäß Angebot (Abschnitt 2) beauftragt:

Pos. Nr.	Leistungsbeschreibung
01	Durchführung einer Prüfung gem. Corona Schnelltest Verfahren in Anlehnung an EN 149:2001+A1:2009 inkl. DEKRA Prüfbericht und Ausstellung eines Konformitätsbewertung Dokuments zum Inverkehrbringen und zur Vorlage bei den Marktaufsichtsbehörden Prüfungsnr.: EN 149:2001+A1:2009, Abschnitte 8.3.2 nur a (Temperaturkonditionierung), 8.3.1 (Gelschussimulation), 8.9.2 und 8.9.3 (Abwasserstand bei Geräte mit und ohne Ventil), 8.3.4 (Austenverfärbungsdurchdringung) und 8.11 (Durchlass des Filtermediums) sowie Schprüfung

Prüfungsverzeichnis nach Abschluss der Prüfungen:

Rücksendung (Die Kosten werden nach Aufwand in Rechnung gestellt)	<input checked="" type="checkbox"/> Ja
Wenn nicht anderweitig vereinbart, werden die Prüfmaterialien 7 Wochen nach Abschluss der Prüfungen vernichtet.	

Ihre Unterschrift: _____ Datum: _____

Projekt-Nr.: _____ Datum: _____

MA&L ENGINEERING GMBH
Semenstr. 15b
40789 Monheim am Rhein
Telefon: +49 212 94000-0
E-Mail: info@mal-engineering.de

DEKRA Testing and Certification GmbH
Hardenbergstr. 15
70565 Stuttgart
Telefon: +49 7141 7801-3480 oder per E-Mail an die Kontaktperson im Anschreiben.

Bitte Rücksendung per Fax: +49 714 7801-3480 oder per E-Mail an die Kontaktperson im Anschreiben.

**Fiscal Year 2020
CERTIFICATION OF REGISTRATION**

This certifies that:

has completed the FDA Establishment Registration and Device Listing with the US Food & Drug Administration, through:

Owner/Operator Number: 10064651
Device Listing#: See annex


This _____ confirm that such registration remains effective upon request and presentation of this certificate until the end of the calendar year stated above, unless said registration is terminated after issuance of this certificate. _____ makes no other representations or warranties, nor does this certificate make any representations or warranties to any person or entity other than the named certificate holder, for whose sole benefit it is issued. This certificate does not constitute an endorsement or approval of the certificate holder's products or establishment by the U.S. Food and Drug Administration. _____ assumes no liability to any person or entity in connection with the foregoing.

Pursuant to 21 CFR 807.65, "Registration of a device establishment or assignment of a registration number does not in any way denote approval of the establishment or its products. Any representation that creates an impression of official approval because a) registration or assignment of a registration number is a labeling or certification requirement." The U.S. Food and Drug Administration does not issue a certificate of registration, nor does the U.S. Food and Drug Administration recognize a certificate of registration. _____ is not affiliated with the U.S. Food and Drug Administration.

FDA

Chief Engineer
Brent M. Mott, D.O.
Expiration Date: December 31, 2020

Web: <http://www.fda.gov> Tel: 1-800-FDA-1088 (1-800-435-6103) Fax: 1-301-793-8345
E-Mail: CDER@fda.hhs.gov E-Mail: CDER@fda.hhs.gov

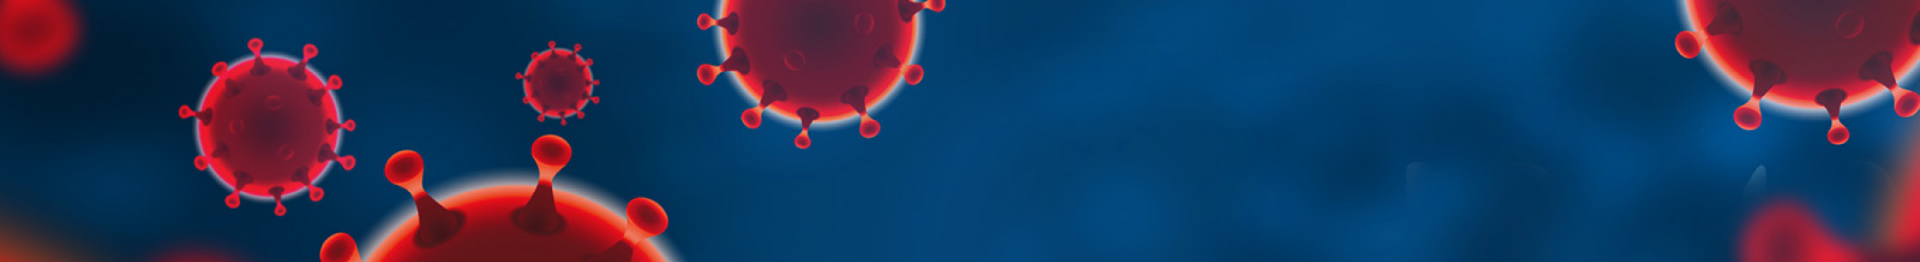


N95 Surgical Particulate-filtering Facial Protection Mask

FDA & CE Approved. MOQ 100K


N95



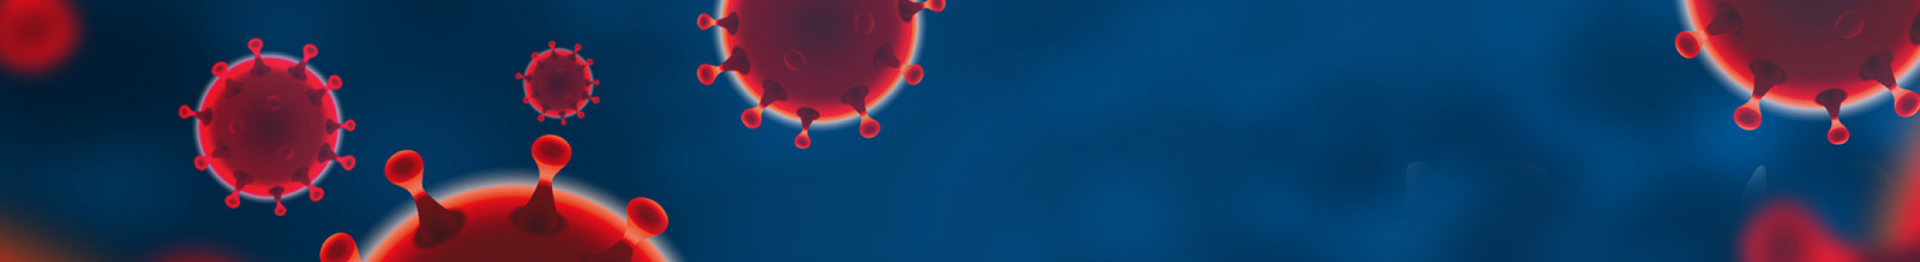


Purchased through registered 3M Distributor

3M 1860 Disposable Particulate Respirator
Surgical Mask – Fluid Resistant
FDA & CE Approved. MOQ 250K
3M 1860

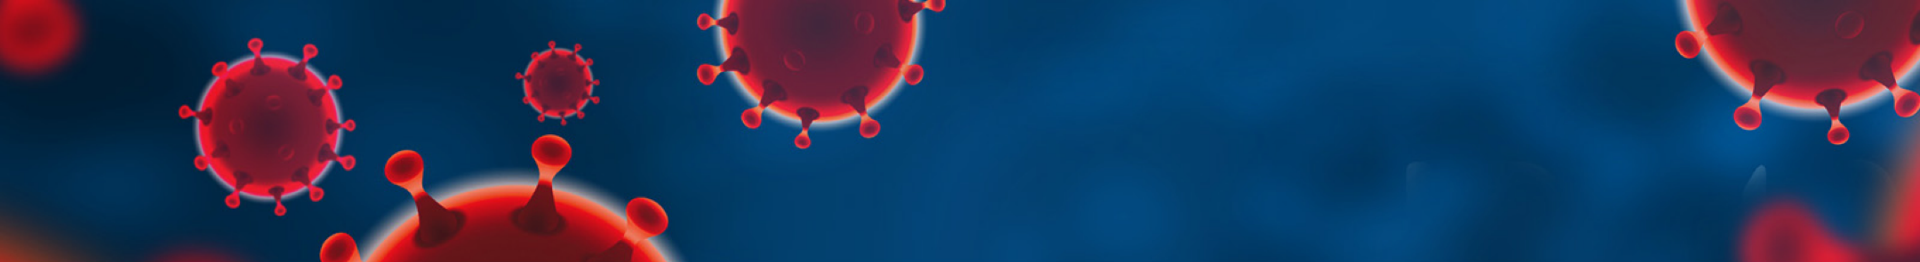


Disposable Gloves Vinyl Examination Rubber
Latex
Powder-Free 100/Box
FDA & CE Approved. MOQ 100K
Gloves




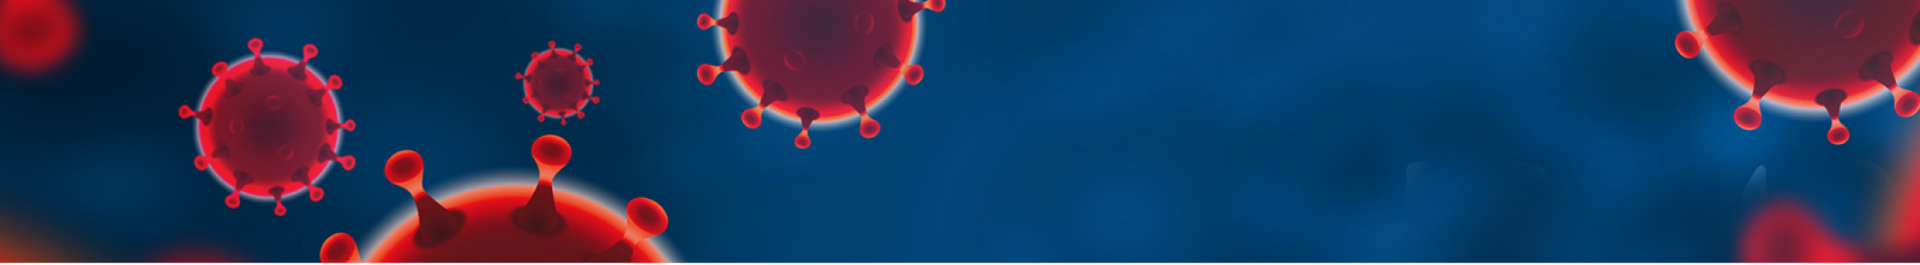

Rapid Test Kits COVID-19 Gold Standard IgG /
IgM Kits
FDA MOQ 50K
Rapid Test Kits

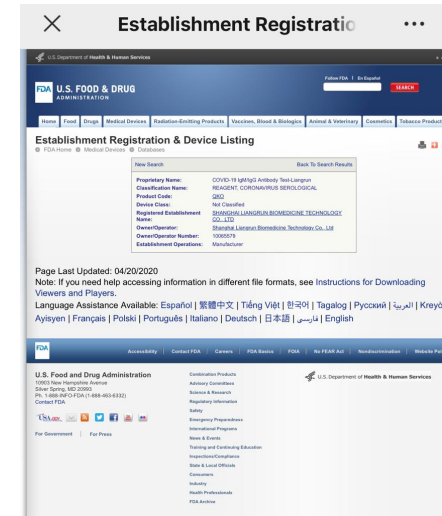

FDA Approved for Marketing & Distribution

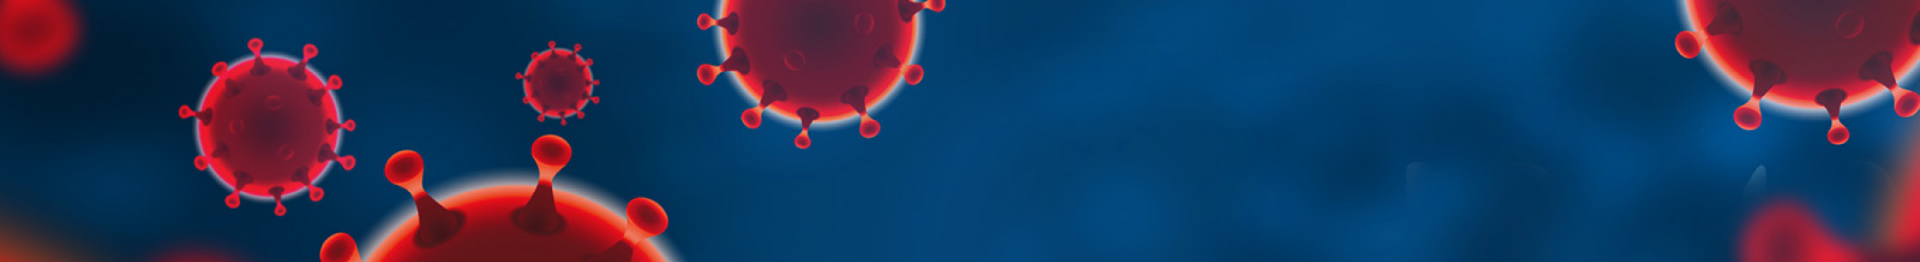

Disposable Isolation Gowns 35-G Waterproof
PP & PE Nonsterile
FDA & CE Approved. MOQ 100K
Isolation Gowns

CIC

CERTIFICATE OF CONFORMITY
EU - Personal protective equipment (PPE)
No. CIC2011T02.2.28

Applicant :
Address :
Manufacturer :
Address :

Product : Protective clothing
Trade Name : MYTT
Model(s) : (2020) 01
Test Report No. : CIC20201702.2.JJ
Test Standards : EN 14126:2003

The tests that have on the above designated product Complies with the essential requirements of Regulation 2016/425 EU.
The test results apply only to the particular sample tested and to the specific tests carried out.
Specifically to the sample investigated in our test reference number only.
The CE markings as shown below can be affixed on the product after preparation of necessary technical documentation.
Other relevant Directives have to be observed.

CE


 HAN ZHOU (China) Engineering
 March 19, 2020

Manufacturer: CIC Testing Technology Co., Ltd.
Add No. 102, Room 1, Building A, No. 28 of Xinhua Road, Xingye Community, Xingye Street,
Huzhou City, Zhejiang Province, China.
Email: info@cic-test.com Tel: 0573-2283247 Fax: 0573-2283247


Fiscal Year 2020
CERTIFICATE OF REGISTRATION

This certifies that :

is registered and has listed the following medical device with the U.S. Food and Drug Administration pursuant to Title 21, § 807 et seq. of the United States Code of Federal Regulations, such registration and listing having been verified as currently effective on, and as of the date hereof.

Registration Number: 3016452400

Code	Device Name
FXP	Shoe Covers
KXA	Face Masks
IMA	Dressing Packs; Procedure Pack
LYU	Surgical Apparel
XME	Bed Sheet
EZO	Liquid Pouches
BYG	Oxygen Masks
OEA	Isolation Gowns
BSJ	Anesthetic Masks
BSY	Suction Catheter
FYF	CAPS

Disclaimer/Disclaimer:
This certificate makes no other representations or warranties, nor does it make any representations or warranties to any person or entity.

FDA




Hand Sanitizer 6.7 FL OZ (200ml)
70% Alcohol with Light Aloe Scent
Transparent Gel/Non-Colored
FDA Approved Facility






Hand Sanitizer 14 FL OZ (415ml)
70% Alcohol with Light Aloe Scent
Transparent Gel/Non-Colored
FDA Approved Facility



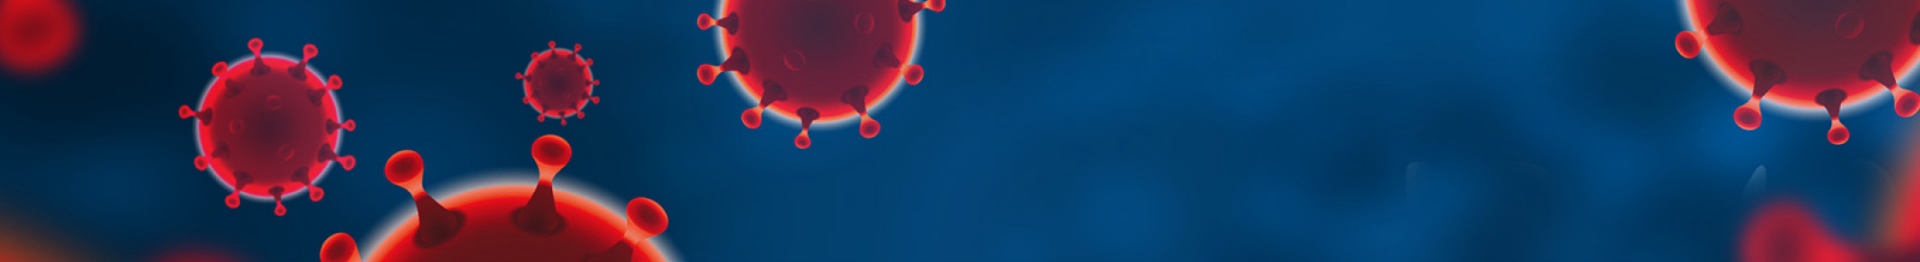

Face Shield Mask
Protects Face and Eyes
Anti-Fog, Waterproof, Anti-Dust
CE, FDA
Face Shield



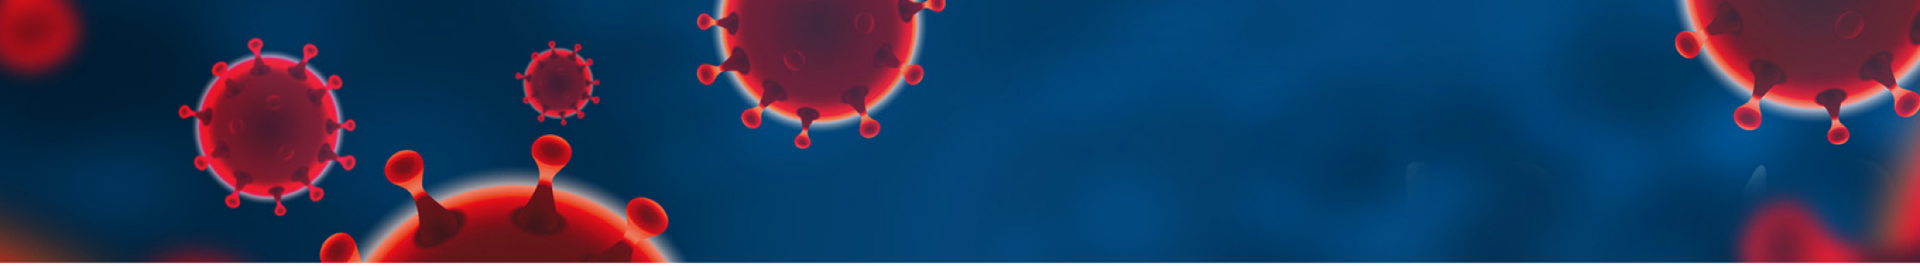

- Customs, duty fees, country tariffs, and regulatory requirements for PPE Imports/Exports vary for each country and can change any day.
- Note: Cost fluctuate day to day. We oversee the logistics and relationship with our manufacturing partners around the globe.
- FOB means cost of item before shipping and fees.
- Average Shipping and fees range \$.20 - \$.30 cents per item

Our Commitment

JR Capital Partners and Z&T Care Solutions in relation with our global partners strive to offer our clients only high quality and certified PPE related products to meet your expectations.



Z&T Care Solutions



JasonRoberts50@Gmail.com

www.JRCapitalPartners.com

